

Corning® Cell Counter

Power of the cloud

CORNING

Accurate Cell Counts in a Flash

For years, the choice between manual and automated cell counting has been a difficult one. Manual cell counting, on the one hand, can be accurate, but time-consuming and very user-dependent. Automated cell counting is much faster and less user-dependent, but the cost of disposable counting slides can be an issue. A tough choice, but now there is a solution.

The Corning Cell Counter is the first automated cell counter that combines the best of both worlds. It is:

- ▶ **Evolving** – periodic, seamless upgrades, added features, and improved functionality.
- ▶ **Accurate** – thanks to its cloud-based machine learning algorithm.
- ▶ **Improved resolution** – most common ability to accurately count as small as 4 μm (e.g., PBMC).
- ▶ **Low-cost** – works with common reusable glass hemocytometers. No consumables required.
- ▶ **Fast** – thanks to its online image processing.

Evolving

Cloud-based processing allows the cell counter to add features and functionality based on user needs, unlike static non-cloud-based cell counters. These updates are efficiently made available to all users at the same time.

Three-second Cell Counts

The Corning Cell Counter can perform a single cell count in less than three seconds*. This is much faster than most automated cell-counting systems. With traditional systems, the image analysis algorithms must be processed on a relatively small onboard computer. The Corning Cell Counter, utilizing the CytoSMART™ Cloud App, can process the images in the Microsoft Azure Cloud Computing Platform. This cloud computing ability means that it can analyze the images faster than any existing onboard processor can.

Higher Accuracy

The Corning Cell Counter uses a cloud-based machine learning algorithm that manages thousands of parameters to provide accuracy without the need to define mammalian cell types. When Trypan Blue is added (Figure 1) the system can also detect cell viability. The Corning Cell Counter can detect clusters of cells, which leads to accurate cell counts of “highly concentrated samples” (up to 1×10^7 cells/mL; Figure 2). The new multicount feature allows multiple images per sample thus increasing overall accuracy.



Improved Resolution

New algorithm allows resolution of mammalian cells as small as 4 μm without an equipment upgrade. For viability, the range is 5 to 70 μm and can accurately count PBMC and CAR-T cells.

Low Cost Like Manual Counting

This cell counter works with the provided counting chamber or customer supplied hemocytometers, enabling users to enjoy the benefits of automated cell counting without the cost of disposable slides. However, for high throughput needs, most major brands of disposable counting chambers are compatible with the Corning Cell Counter.

Easy to Use

The Corning Cell Counter is easy to use. Simply connect the cell counter to your computer or tablet and start the CytoSMART Cloud App. Place the loaded counting chamber on the stage. Focus on your cells and press the Count button. The simplicity of the cell counter allows anyone working in your lab to easily count cells without the need of extensive training.

*Measured using a 73 Mbps download speed and a 20 Mbps upload speed. Actual speed can vary depending on the internet connection.

Accessible Data Anywhere, Anytime

With the Corning® Cell Counter, the report is instantly shown on your computer and sent to the CytoSMART™ Cloud App, enabling you to look up the analyzed image and cell count on your smartphone, tablet, or computer. Since all data is saved in the CytoSMART Cloud App, you can gain insight into the health and quality of your cell culture from one experiment to the next.

Specifications

Counting range	5×10^4 to 1.0×10^7 cells/mL
Counting range	4 to 70 μm ; 5 to 70 μm with viability
Measurement time	<3 sec.*
Compatibility	Reusable and disposable counting chambers
Sample volume	10 μL
Weight	1.0 kg
Multicount capability	Maximum of 8
Field of view	2.0 x 1.5 mm or 1.39 x 1.39 mm
Magnification	200X
Image resolution	2048 x 1536
Exported formats	PNG
Light source	LED
Camera	5 MP CMOS
Unit dimensions	122 x 122 x 125 (L x W x H)
Operating environment	5°C to 40°C, 20% to 95% humidity

*Measured using a 73 Mbps download speed and a 20 Mbps upload speed. Actual speed can vary depending on the internet connection.

Ordering Information

Cat. No.	Description	Qty/Cs
6749	Corning Cell Counter	1
480200	Counting Chamber	1

Contact your local Corning Account Manager to request a demonstration of the Corning Cell Counter.

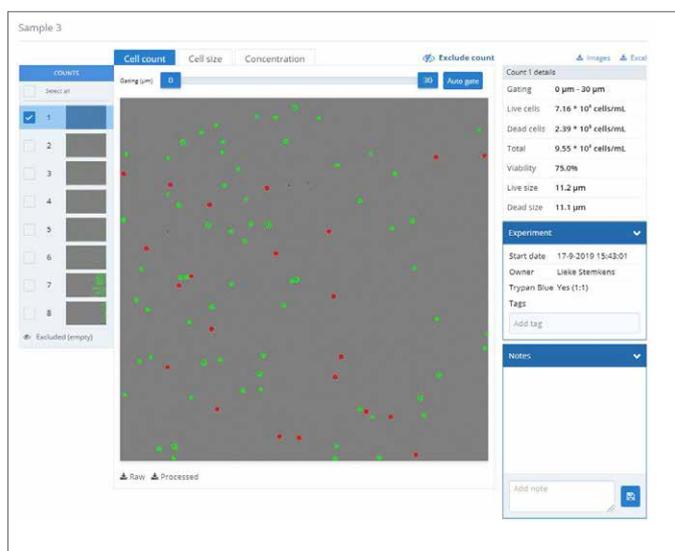


Figure 1. Results page after performing multiple counts with the Version 3 algorithm. In the top left the sample name is displayed. Underneath this you can see the tutorial button, the counts taken of this sample, and the dilution calculator. The box on the top right contains details of the count. General information is displayed in the “Experiment” box, while notes can be added in the “Notes” box.

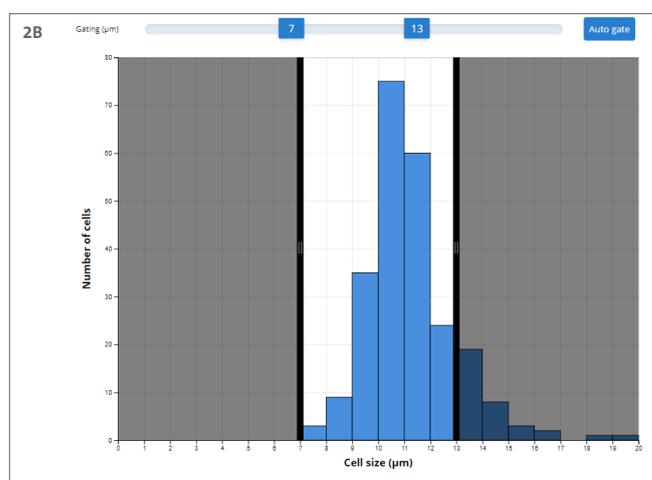
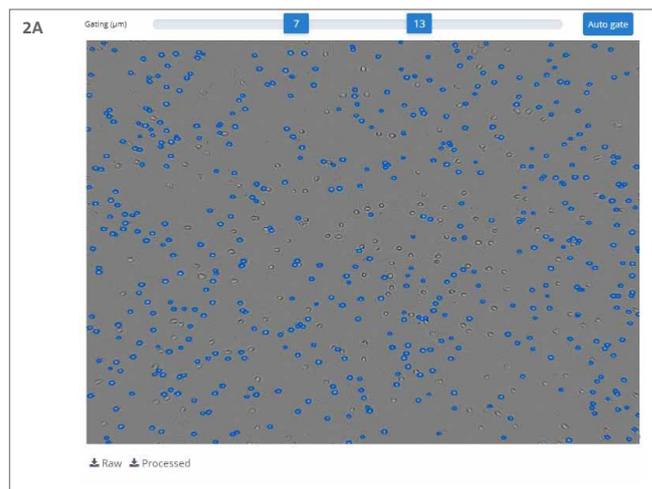


Figure 2. Example of live gating using the gating slider. The minimum and maximum are set on 7 and 13 μm , respectively. (A) Live gating in the “Cell count” tab. Cells that are smaller than 7 μm or larger than 13 μm are not encircled in blue. (B) Live gating in the “Cell size” tab. The shaded regions represent the excluded values.

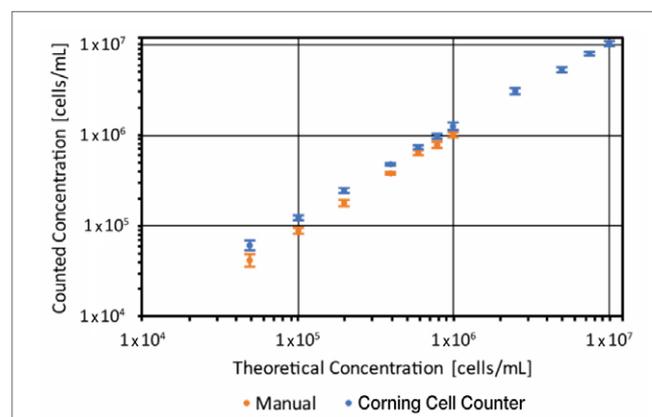


Figure 3. Different concentrations of C6 cells were counted manually and using the Corning Cell Counter (n = 3). In both cases, the count corresponds well with the theoretical concentration (error bars represent the standard deviation).

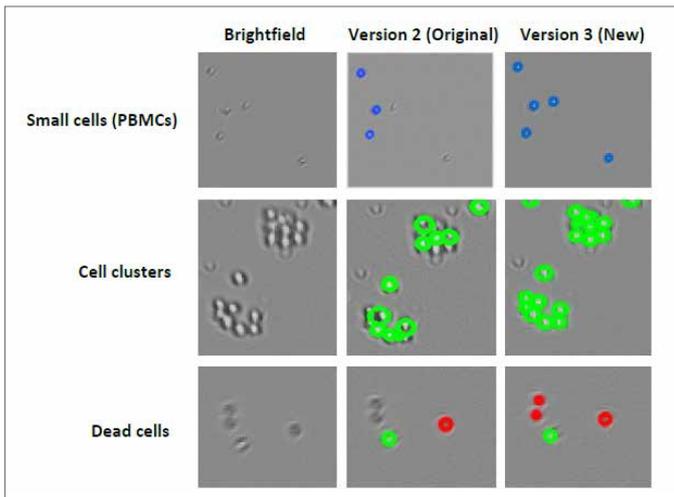


Figure 4. Visualization of the improvements of the Version 3 algorithm. The columns (from left to right) represent the Brightfield images, the Version 2 (Original) processed image, and the Version 3 processed image, respectively. The rows (from top to bottom) represent samples that contain small cells, cell clusters, or dead cells, respectively.

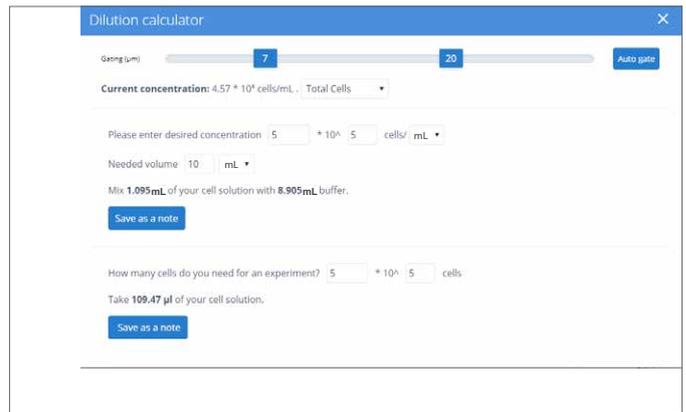


Figure 6. Dilution calculator. The dilution calculator can be used for several purposes. A user can enter the concentration they need in a certain volume using the values of the live/dead/total cell concentrations. It also calculates how much volume of the counted cell suspension is required for a certain number of cells.

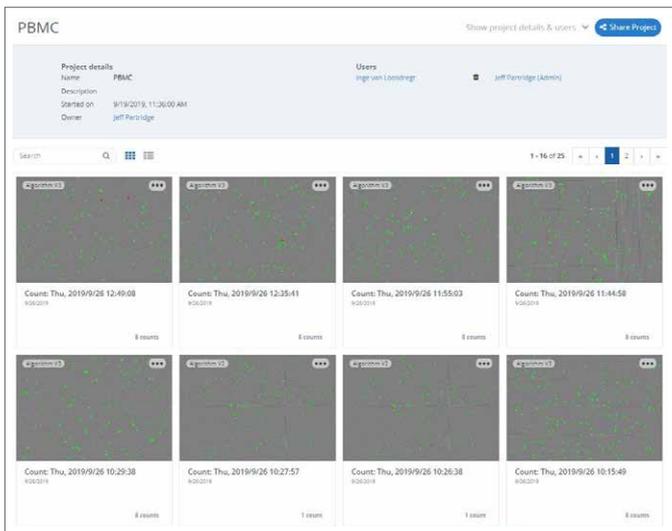


Figure 5. Look back at your data on the CytoSMART Cloud App.

For more specific information on claims, visit the Certificates page at www.corning.com/lifesciences.

Warranty/Disclaimer: Unless otherwise specified, all products are for research use only. Not intended for use in diagnostic or therapeutic procedures. Corning Life Sciences makes no claims regarding the performance of these products for clinical or diagnostic applications.

CORNING

Corning Incorporated Life Sciences

836 North St.
Building 300, Suite 3401
Tewksbury, MA 01876
t 800.492.1110
t 978.442.2200
f 978.442.2476

www.corning.com/lifesciences

ASIA/PACIFIC

Australia/New Zealand
t 61 427286832

Chinese Mainland
t 86 21 3338 4338
f 86 21 3338 4300

India
t 91 124 4604000
f 91 124 4604099

Japan

t 81 3-3586 1996
f 81 3-3586 1291

Korea

t 82 2-796-9500
f 82 2-796-9300

Singapore

t 65 6572-9740
f 65 6735-2913

Taiwan

t 886 2-2716-0338
f 886 2-2516-7500

EUROPE

CSEurope@corning.com

France

t 0800 916 882
f 0800 918 636

Germany

t 0800 101 1153
f 0800 101 2427

The Netherlands

t 020 655 79 28
f 020 659 76 73

United Kingdom

t 0800 376 8660
f 0800 279 1117

All Other European Countries

t +31 (0) 206 59 60 51
f +31 (0) 206 59 76 73

LATIN AMERICA grupoLA@corning.com

Brazil

t 55 (11) 3089-7400

Mexico

t (52-81) 8158-8400

For additional product or technical information, visit www.corning.com/lifesciences or call 800.492.1110. Outside the United States, call +1.978.442.2200 or contact your local Corning sales office.